This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.



Replacement Drawing Sheet
WHITENING TIP FOR DENTAL FLOSSING DEVICE
Application No: 10/750,720; Filed: December 31, 2003;
Atty. Docket No.: 456902-521/2056/US/2

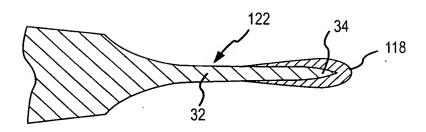


FIG.21A

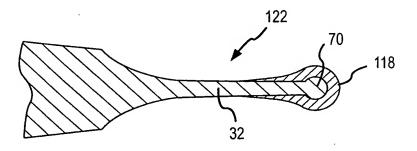


FIG.21B

13/25




FIG.22A




FIG.22B

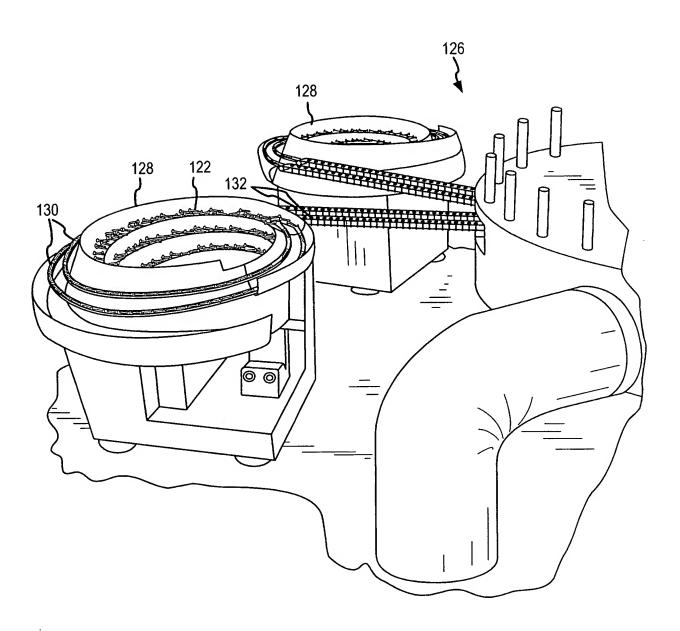


FIG.23

15/25

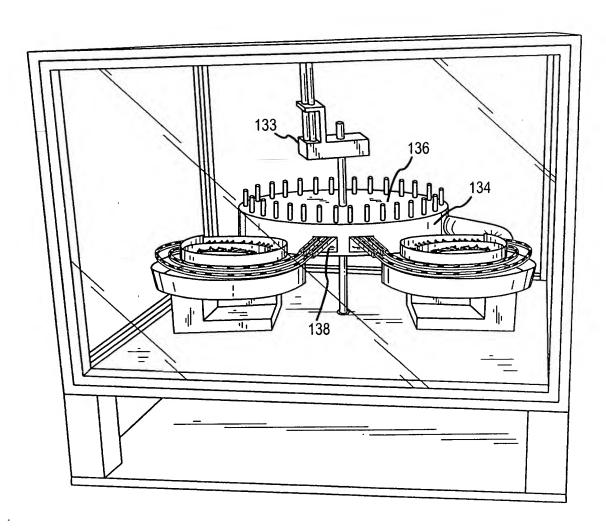


FIG.24

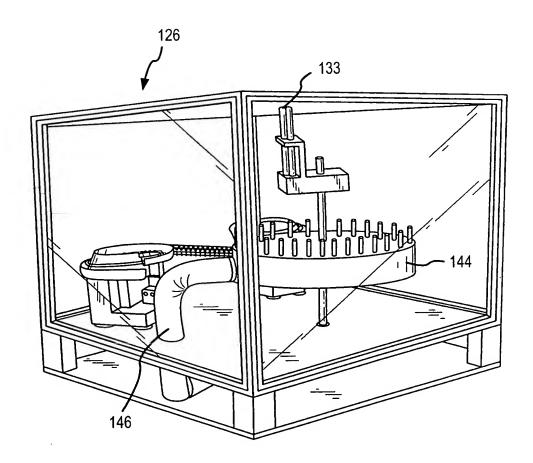


FIG.25

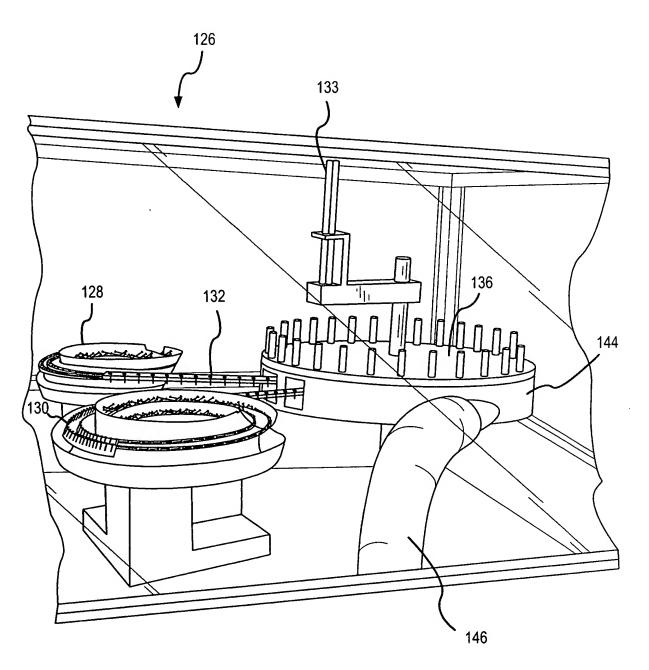


FIG.26

18/25

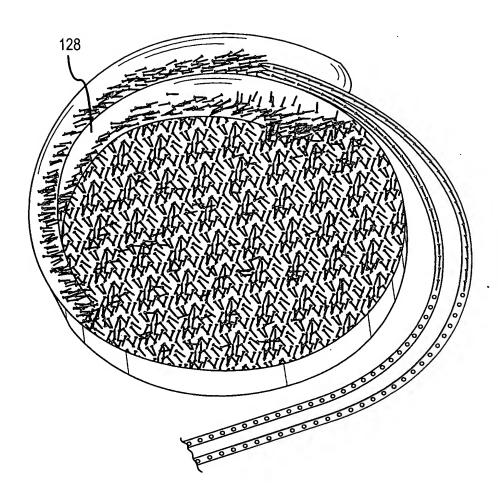


FIG.27

19/25

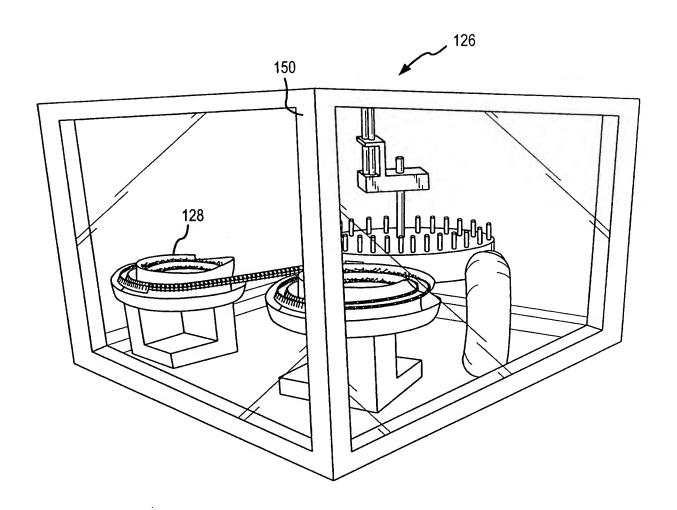


FIG.28

20/25

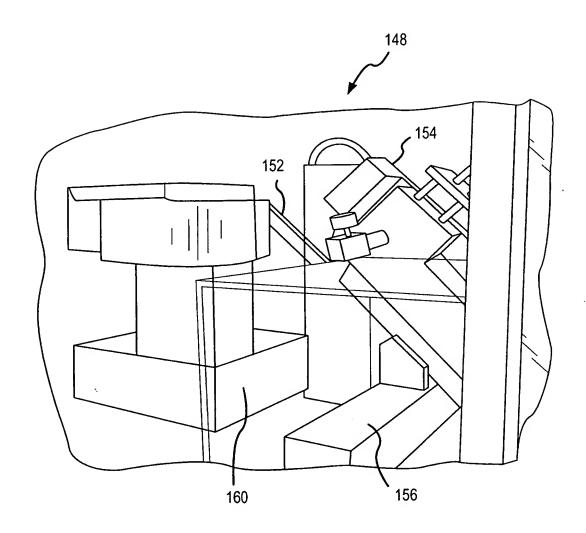


FIG.29

21/25

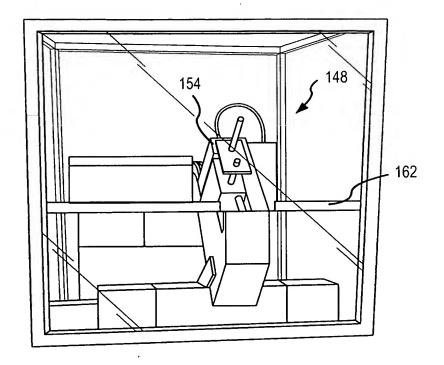


FIG.30

22/25

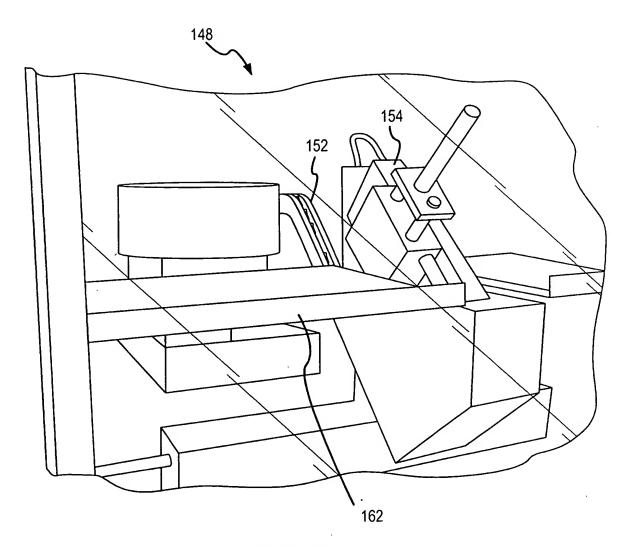


FIG.31

23/25

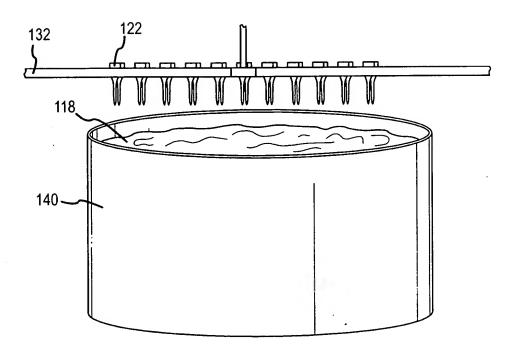


FIG.32

24/25

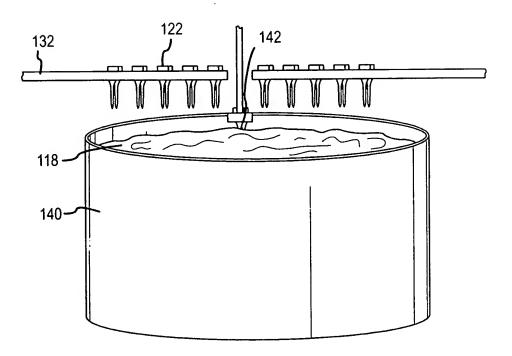


FIG.33A

25/25

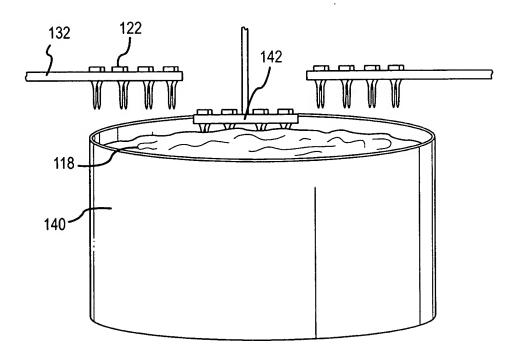


FIG.33B